



US 20140125338A1


(19) **United States**(12) **Patent Application Publication**
KRZYZAK(10) **Pub. No.: US 2014/0125338 A1**(43) **Pub. Date: May 8, 2014**(54) **ANISOTROPIC DIFFUSION PHANTOM FOR
CALIBRATION OF DIFFUSION TENSOR
IMAGING PULSE SEQUENCES USED IN MRI**(71) Applicant: **Artur KRZYZAK**, Krakow (PL)(72) Inventor: **Artur KRZYZAK**, Krakow (PL)(21) Appl. No.: **14/156,493**(22) Filed: **Jan. 16, 2014****Related U.S. Application Data**(63) Continuation of application No. 12/994,760, filed on
Nov. 25, 2010, now Pat. No. 8,643,369, filed as appli-
cation No. PCT/PL2009/000051 on May 19, 2009.(30) **Foreign Application Priority Data**

May 26, 2008 (PL) P.385276

Publication Classification(51) **Int. Cl.**
G01R 33/58 (2006.01)(52) **U.S. Cl.**
CPC **G01R 33/58** (2013.01)
USPC **324/318**(57) **ABSTRACT**

The subject matter of the invention concerns the anisotropic diffusion phantom for the calibration of any diffusion MR-DTI imaging sequence and a method for the calibration of all the MRI scanners by using anisotropic diffusion models based on the “b” matrix, which is a quantity specific for every

magnetic resonance (MR) imaging sequence and the MRI scanner used. It has application in the study of solids, amorphous materials, liquids and biological tissues. The anisotropic diffusion phantom for the calibration of any MR imaging sequence is any anisotropic diffusion model of any shape for the hydrogen H_2 contained in H_2O or LC, for example. The diffusion standard according to the invention is preferably a pipe with a bundle of capillaries filled with H_2O , hydrogel or any other substance that contains hydrogen nuclei or any volume, preferably cylindrical, filled with H_2O , hydrogel or any other substance that contains hydrogen nuclei or densely filled with non-magnetic cylindrical rods free of hydrogen nuclei. In another embodiment, the diffusion model is an array of thin glass plates (1) separated with layers of H_2O , hydrogel or any other substance that contains hydrogen nuclei (2). The model, being a pipe with a bundle of capillaries, has the capillaries selected so that the restriction of diffusion at a temperature in the direction perpendicular to the capillary axis is significant with respect to the range of diffusion times Δ in the diffusion MR imaging sequence. For the calibration of any MR imaging sequence using the anisotropic diffusion phantom of the invention, the anisotropic diffusion phantom is placed in the volume of the MRI scanner tested. Subsequently, the number of “b” matrices needed for the calculation of the diffusion tensor is determined based on the anisotropic diffusion model. This constitutes no less than six “b” matrices as defined spatially for each voxel and for the specific directions of the diffusion gradient vector. Therefore, in the simplest case, 36 “b” matrices and one “b₀” matrix without diffusion gradients are determined. The anisotropic diffusion phantom is a diffusion model for which the diffusion tensor in the system of principal axes assumes known values. The diffusion model is rotated by various Euler angles, so that the determinant D_M of the matrix whose columns correspond to the components of the diffusion tensor D is different from zero after each rotation.

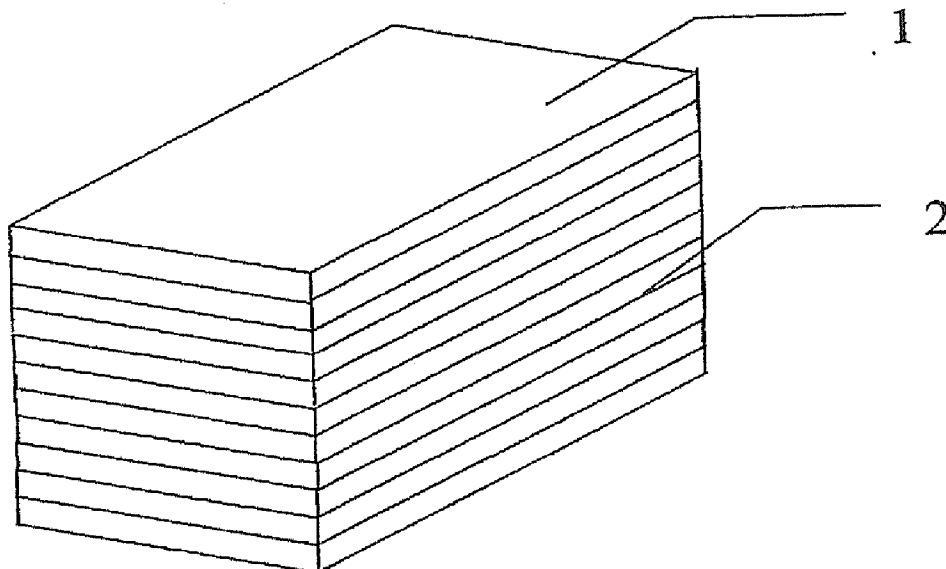

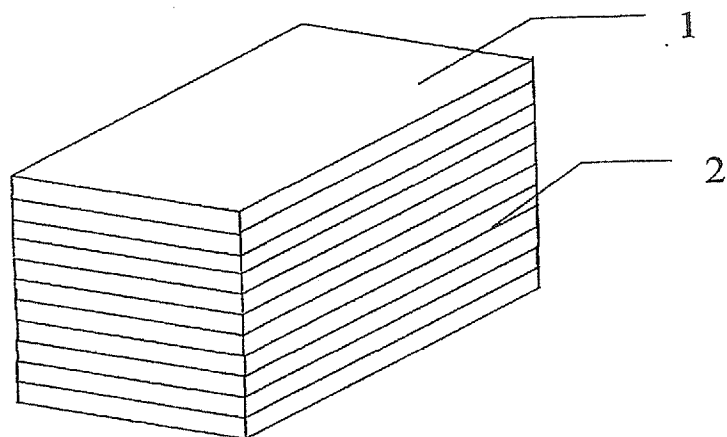


Fig.1.

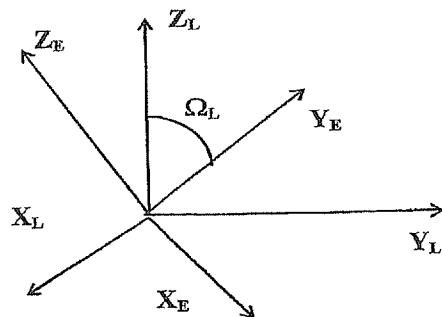


Fig.2.

ANISOTROPIC DIFFUSION PHANTOM FOR CALIBRATION OF DIFFUSION TENSOR IMAGING PULSE SEQUENCES USED IN MRI

BACKGROUND

[0001] The subject matter of the invention concerns the anisotropic diffusion phantom for the calibration of any diffusion MR-DTI imaging sequence and a method for the calibration of any Magnetic Resonance Imaging (MRI) scanner by using anisotropic diffusion models based on the b'' matrix, which is a quantity specific for every magnetic resonance (MR) imaging sequence and MRI scanner that are used, employed in the examination of biological tissues, solids, amorphous materials and liquids.

[0002] In the prior art, the values of the $\Delta^2 b''$ matrix that were needed to calculate the diffusion tensor were determined analytically and separately for every diffusion MR imaging sequence and MRI scanner; the results were approximate only due to the complex formulae used in the calculation. Alternatively, a single value of the $\approx 80^\circ b''$ matrix that was assumed for the entire volume of the object in question was used for the calculation of the diffusion tensor

BRIEF DESCRIPTION OF DRAWINGS

[0003] Attention is now directed to the drawings, where like reference numerals or characters indicate corresponding or like components. In the drawings:

[0004] FIG. 1 shows an outline of an anisotropic diffusion phantom in accordance with an embodiment of the invention; and

[0005] FIG. 2 is a diagram of a laboratory reference system.

DETAILED DESCRIPTION OF THE DRAWINGS

[0006] A disadvantage of the diffusion tensor calculation methods known in the art is the large contribution of calculation errors as the approximate “ b'' ” matrix values are used and a lack of any spatial distribution of the b'' matrix is assumed. Therefore, it is rather difficult to determine the water diffusion fluctuations in the object examined by using an MRI scanner properly, precisely and quantitatively, and the reproducibility of the results is non-existent. Distinct MR sequences occur for various MRI scanners; in consequence, the results are discrepant and hardly comparable. The results are fraught with errors as it is impossible to precisely determine the “ b'' ” matrix values.

[0007] The following acronyms will be used throughout the document:

[0008] MR—Magnetic Resonance

[0009] DTI—Diffusion Tensor Imaging

[0010] LC—Liquid Crystal

[0011] A calibration method of the invention for any MRI scanner eliminates these shortages and enables the precise and spatial determination of “ b'' ” matrix values for any MRI scanner and any imaging sequence, in particular DTI.

[0012] In the method of the invention, the “ b'' ” matrix is determined precisely based on the anisotropic diffusion model, for each voxel of the volume tested.

[0013] The anisotropic diffusion phantom for the calibration of any MR imaging sequence of the invention is any anisotropic diffusion model of any shape for the hydrogen contained in H_2O or in LC, for example. The diffusion model according to the invention is preferably a pipe with a bundle of capillaries filled with H_2O , hydrogel or any other substance

that contains hydrogen. Other 3D shapes, preferably cylindrical, filled with densely non-magnetic cylindrical rods without hydrogen nuclei could be regarded as a reference diffusion model as well. The rods are preferably made of glass, Teflon or any other material with similar properties. They are immersed in H_2O , hydrogel or any other substance that contains hydrogen nuclei. In one embodiment, the diffusion model is an array of thin glass plates separated by the layers of H_2O , hydrogel or any other substance that contains hydrogen nuclei. The diffusion model can also be formed by anisotropic liquid crystals (LC) or others for other elements that may be used in imaging in future, such as for example 2H , 3He , ^{13}C , ^{14}N , ^{17}O , ^{19}F , ^{29}Si , ^{31}P , etc. The model, being a pipe with a bundle of capillaries, has the capillaries selected so that the restriction of diffusion at a temperature in the direction perpendicular to the capillary axis is significant with respect to the range of diffusion times Δ in the diffusion MR imaging sequence. For the diffusion model filled with water at ambient temperature, it is within a range of 0.1 μm to 100 μm . For hydrogel, the values are lower. The free diffusion of water molecules across the capillaries or across the cylindrical rods or perpendicularly to the plane of the thin glass plates is inhibited by the opposite capillary or rod wall or by the plane of the opposite thin glass plate and restricts the diffusion process. By adjusting the capillary diameters, cylindrical rod diameters or the thickness of the layers of H_2O , hydrogel or any other substance that contains hydrogen nuclei between thin glass plates, the diffusion limit is determined for specified diffusion times Δ and temperature T based on the fact that free diffusion is given by the Einstein-Smoluchowski equation:

$$\langle (\mathbf{P} - \mathbf{P}_o)(\mathbf{P} - \mathbf{P}_o) \rangle = 6D\Delta t \quad [1]$$

where:

\mathbf{P} —position vector of the diffusing molecule at time t ,

\mathbf{P}_o —initial position vector.

The equation determines the relation between the average square of the path and the diffusion coefficient D .

[0014] The anisotropic diffusion model in the system of principal axes has no less than two distinct diffusion tensor components, wherein for the phantom made of a bundle of capillaries it is a symmetrical diffusion tensor D :

$$\begin{pmatrix} D_{xx} & D_{xy} & D_{xz} \\ D_{yx} & D_{yy} & D_{yz} \\ D_{zx} & D_{zy} & D_{zz} \end{pmatrix}$$

which obtains the following form after diagonalisation in the system of the principal axes:

$$\begin{pmatrix} D_1 & 0 & 0 \\ 0 & D_2 & 0 \\ 0 & 0 & D_3 \end{pmatrix}$$

where:

[0015] D_{ij} —components of the symmetrical diffusion tensor in the laboratory system,

[0016] D_1, D_2 —diffusion coefficients determined in the transverse direction of the capillary,

[0017] D_3 —diffusion coefficient in the longitudinal direction of the capillary.

[0018] In the case in question: $D_1=D_2$ and $D_2 \neq D_3$.

In the present invention, the anisotropic diffusion model is determined as follows:

[0019] typical one dimensional experiments are carried out for the measurement of the diffusion coefficients for the anisotropy directions in order to determine e.g. D_1, D_2 and D_3 depending on the diffusion time and temperature. Thus, an anisotropic diffusion model is obtained, being a function of temperature T and diffusion time Δ .

[0020] Any MRI scanner can be calibrated by using the method of the invention in order to measure the “b” matrix precisely and spatially. It leads consequently into a precise measurement of the diffusion tensor assuming that in biological tissues it is primarily the water diffusion tensor.

[0021] The diffusion tensor is measured according to the known formula:

$$\ln\left(\frac{A(b)}{A(0)}\right) = - \sum_{i=1}^3 \sum_{j=1}^3 b_{ij} D_{ij} \quad [2]$$

where:

[0022] $A(b)$ —echo signal (MR image intensity), measured for each voxel,

[0023] $A(0)$ —MR image intensity for $b=0$

[0024] b_{ij} —element of the symmetrical “b” matrix,

[0025] b_{ij} —element of the symmetrical diffusion tensor D .

[0026] It follows from formula [2] that for the DTI experiments, in order to calculate the water diffusion tensor, wherein the symmetrical tensor is a 3×3 matrix, no less than seven MR experiments need to be carried out, for which the MR sequences shall contain six distinct non-collinear directions of diffusion gradients and one (the seventh) direction without diffusion gradients applied. Hence, for the simplest DTI experiment, no less than six symmetrical “b” matrices, each of which contains six distinct components, are determined for each diffusion gradient vector.

[0027] For the calibration of any MR imaging sequence by using the anisotropic diffusion phantom of the invention, the anisotropic diffusion phantom is placed inside the volume of the MRI scanner tested. Subsequently, the number of “b” matrices needed for the calculation of the diffusion tensor is determined based on the anisotropic diffusion model. This constitutes no less than six “b” matrices to be defined spatially for each voxel and for the specific directions of the diffusion gradient vector. Therefore, in the simplest case, 36 “b” matrices and one “ b_0 ” matrix—without diffusion gradients—are determined.

[0028] In order to determine the value of the “b” matrix for the direction of the diffusion gradient vector, a system of no less than six equations is solved for the distinct diffusion tensor D values. For a diffusion gradient vector direction, a diffusion tensor value is used based on the specified diffusion model for the diffusion time Δ and the temperature of the respective experiment. Various diffusion model tensor values

are preferably obtained by rotating the anisotropic diffusion phantom inside the MRI scanner volume in question. The anisotropic diffusion phantom is a diffusion model for which the diffusion tensor in the system of the principal axes assumes known values. The diffusion model is rotated by various Euler angles, so that the determinant D_M of the matrix, whose columns correspond to the components of the diffusion tensor D is different from zero after each rotation.

$$\det(D_M) \neq 0$$

The following matrix is derived in the measurements:

$$D_M = \begin{pmatrix} D_{11} & D_{12} & D_{13} & D_{14} & D_{15} & D_{16} \\ D_{21} & D_{22} & D_{23} & D_{24} & D_{25} & D_{26} \\ D_{31} & D_{32} & D_{33} & D_{34} & D_{35} & D_{36} \\ D_{41} & D_{42} & D_{43} & D_{44} & D_{45} & D_{46} \\ D_{51} & D_{52} & D_{53} & D_{54} & D_{55} & D_{56} \\ D_{61} & D_{62} & D_{63} & D_{64} & D_{65} & D_{66} \end{pmatrix},$$

where for D_{ij} :

[0029] i —successive components of the diffusion tensor:

xx, yy, zz, xy, xz, yz,

[0030] j —in the range of 1 to 6—successive sets of Euler angles.

For the calculation of the “b” matrix values for a direction of the diffusion gradient vector, the following system of equations is solved, derived from equation [2]:

$$L = b D_M, \quad [3]$$

where:

[0031] b —six calculated components of the “b” matrix converted into the vector form,

[0032] D_M —matrix whose columns are formed by the components of the model diffusion tensor after successive rotations by various Euler angles,

[0033] L —successive

$$\ln\left(\frac{A(b)}{A(0)}\right)$$

values from measurements (based on MR images) converted into the form of a transposed vector.

The system of equations [3] is solved for the remaining (no less than six non-collinear) directions of diffusion gradients. Thus, 36 “b” matrices and a “ b_0 ” matrix are derived. Therefore, the “b” matrix values are obtained for the specific directions of diffusion gradients and for each voxel of the volume in question.

[0034] Based on the calibration method of the invention, a diffusion model for the volume examined is formed and selected for an RF coil depending on its shape and parameters. The calibration is repeated every time before the change of the imaging sequence parameters, in particular when changing the diffusion gradients.

[0035] The advantage of the calibration method for any MRI scanner using anisotropic diffusion models based on the anisotropic diffusion phantom for the calibration of any diffusion MR-DTI imaging sequence is the precise and spatial determination of the “b” matrix value. As a result it is possible, contrary to the prior art, to precisely measure the diffusion tensor, first of all in biological systems, but also in

other systems. Furthermore, the calibration method provides a real possibility to compare the diffusion tensor values for the objects tested, which are derived by using various MRI scanners and distinct MR imaging sequences.

EXAMPLE

[0036] The following operations were performed for the calibration of an MSED (Multislice Spin Echo Diffusion) sequence in an MRI scanner with a superconducting magnet (field intensity: 4.7 T) by using an anisotropic diffusion model at T=21° C. and diffusion time $\Delta=50$ ms:

[0037] 1. An anisotropic diffusion phantom in the form of an array of thin glass plates separated with H₂O layers (thickness: 10 μ m) was placed in an MRI scanner with a superconducting magnet (field intensity: 4.7 T) in the influence area of a 3 cm birdcage RF coil. Tomographic measurements were carried out by using an MSED sequence.

[0038] 2. MR tomographic measurements for the determination of the spatial “b” matrix for one direction of the diffusion gradient vector were carried out for six distinct positions defined by the rotation of the anisotropic diffusion phantom by Euler angles. The entire measurement volume tested in the MRI scanner in the interaction area of the RF coil was scanned to obtain the spatial distribution of the “b” matrix. The measurements were repeated for further diffusion gradient vector directions. A total of 36 MR measurements were carried out in six distinct diffusion gradient vector positions and an additional scan for the diffusion gradient vector=0.

[0039] 3. Subsequently, the operations in steps 1 and 2 were repeated for the other sequence parameters; as a result, a digital record of the spatial “b” matrix values was derived that corresponded to various imaging sequence parameters. The “b” matrix values, thus obtained, enabled the precise calculation of the diffusion tensor by using a DTI sequence in the parameter range for which the “b” matrix value was determined.

[0040] The anisotropic diffusion phantom and calibration method for any MR imaging sequence according to the embodiment is shown in the figure, wherein FIG. 1 shows the outline of the anisotropic diffusion phantom in the form of an array of thin glass plates separated with H₂O layers and FIG. 2 shows the phantom (diffusion model) rotation method by successive Euler angles.

[0041] The anisotropic diffusion phantom is made from thin glass plates 1, each of which is separated with a 10 μ m H₂O layer 2. The system of principal axes (E) shown in FIG. 2 is the laboratory reference system (L) related to the diffusion model after rotation and their mutual orientation as defined by the Euler angles

$$\Omega_L=(\alpha_L, \beta_L, \gamma_L).$$

Due to the symmetry, the diffusion tensor measured in the laboratory system (L) has 6 components different from zero. In the system of principal axes (E), the diffusion tensor is defined by three principal components and three Euler angles Ω_L . For a known tensor in the system of principal axes (E) and

known Euler angles, the tensor values in the laboratory system (L) are determined by a rotation transformation $R(\alpha_L, \beta_L, \gamma_L)$ according to the formula:

$$D_L=R^{-1}(\Omega_L)D_ER(\Omega_L)$$

where:

[0042] $R(\Omega_L)$ —Wigner rotation matrix,

[0043] $\Omega_L=(\alpha_L, \beta_L, \gamma_L)$ —Euler angles that define the orientations of the system of principal axes (E) with respect to the laboratory system (L),

[0044] D_L, D_E —diffusion tensors in L and E systems, respectively.

[0045] The diffusion model is rotated by various Euler angles, so that the determinant D_M of the matrix, whose columns correspond to the components of the diffusion tensor D, is different from zero after each rotation.

$$\det(D_M) \neq 0$$

1. An anisotropic diffusion phantom forming a model for the calibration of an MR-DTI imaging sequence for an MR scanner at a specified temperature for a specified range of diffusion times, characterised in that it is formed by a volume densely filled with non-magnetic elements (1) aligned in parallel to at least one common parallel alignment axis and a substance (2) that contains hydrogen nuclei, the non-magnetic elements (1) and the substance (2) arranged such that diffusion of the substance (2) that contains hydrogen nuclei is significantly restricted in the direction perpendicular to the parallel alignment axis for the specified temperature with respect to the specified range of diffusion times.

2. The anisotropic diffusion phantom according to claim 2, wherein the non-magnetic elements form a bundle of capillaries filled with the substance (2) that contains hydrogen nuclei.

3. The anisotropic diffusion phantom according to claim 2, wherein the non-magnetic elements form a bundle of rods surrounded by the substance (2) that contains hydrogen nuclei.

4. The anisotropic diffusion phantom according to claim 2, wherein the non-magnetic elements form an array of thin plates (1) between which the substance (2) that contains hydrogen nuclei is located.

5. The anisotropic diffusion phantom according to claim 2, wherein the substance (2) that contains hydrogen nuclei is H₂O or hydrogel.

6. The anisotropic diffusion phantom according to claim 2, wherein the substance (2) that contains hydrogen nuclei comprises liquid crystals (LC).

7. The anisotropic diffusion phantom according to claim 2, wherein the substance (2) that contains hydrogen nuclei comprises a substance containing ²H, ³He, ¹³C, ¹⁴N, ¹⁷O, ¹⁹F, ²⁹Si, ³¹P etc.

8. The anisotropic diffusion phantom according to claim 2, wherein the non-magnetic elements are made of glass or Teflon.

9. The anisotropic diffusion phantom according to claim 2, wherein the non-magnetic elements are free of hydrogen nuclei.

* * * * *